




Results from the Norwegian Arthroplasty Register



HACTIV cementless stem

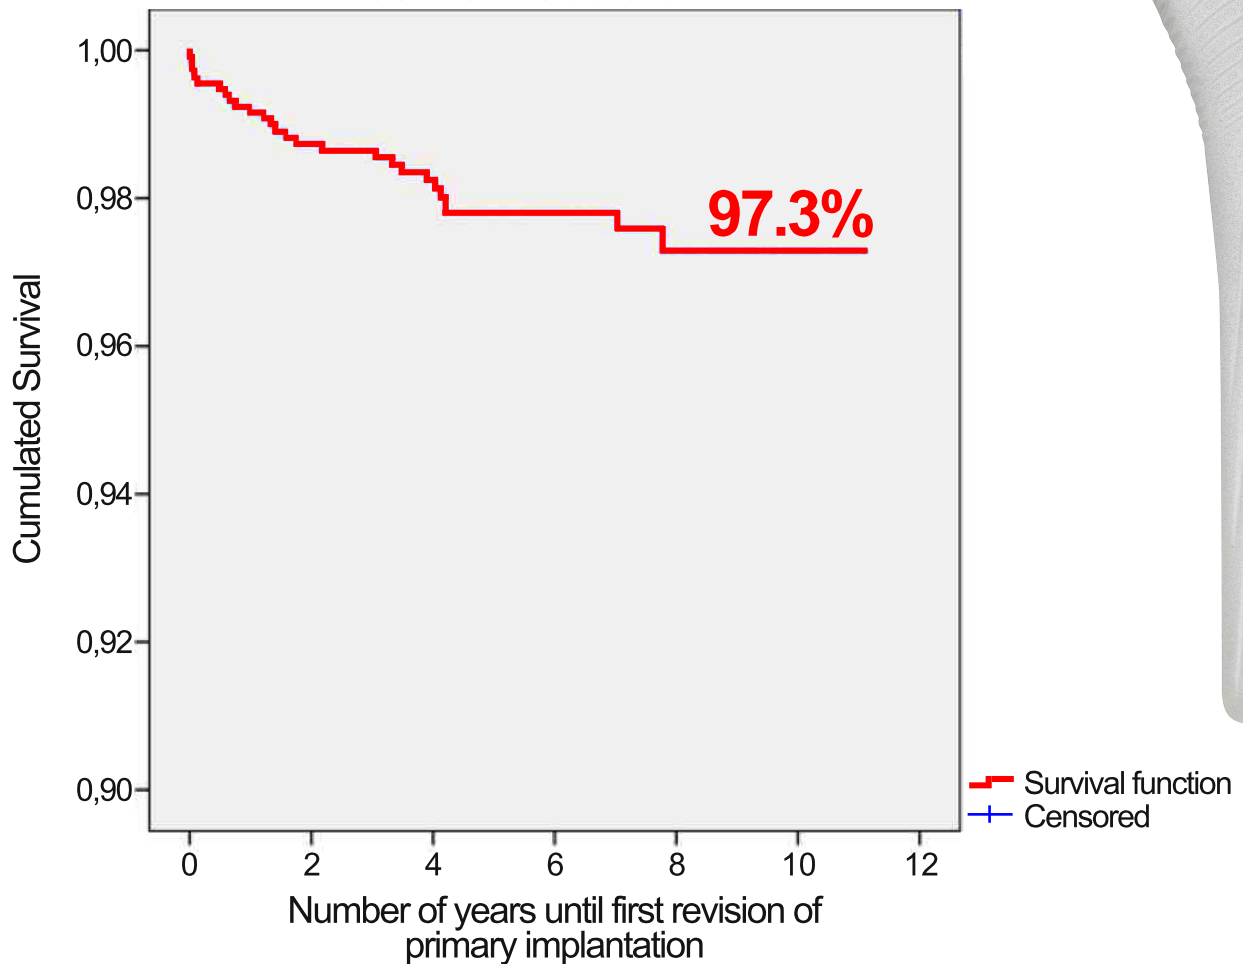

1350 HACTIV cementless prosthesis implanted
27 prosthesis revised

97.3%*
of success at
10 years

* 95% Confidence Interval: [96.1 - 98.5] - NAR 2013 data analysis